

Legend


Important notes

The authors and Erbe Elektromedizin GmbH have taken the greatest possible care while compiling the catalogue with electrosurgical accessories. Nevertheless, it is impossible to exclude the possibility that errors may be contained herein.

The information and recommendations given here may not be construed as constituting any basis for any claims against Erbe Elektromedizin GmbH. Should legal regulations stipulate liability, such liability shall be limited to intentional misconduct or gross negligence.

The data on the use of instruments is based on clinical experience. Medical science is subject to a process of permanent change based on research and clinical experience. Therefore the products are subject to alterations in design and technique. Because of production tolerances dimensions in the catalogue may marginally differ.

Further product information

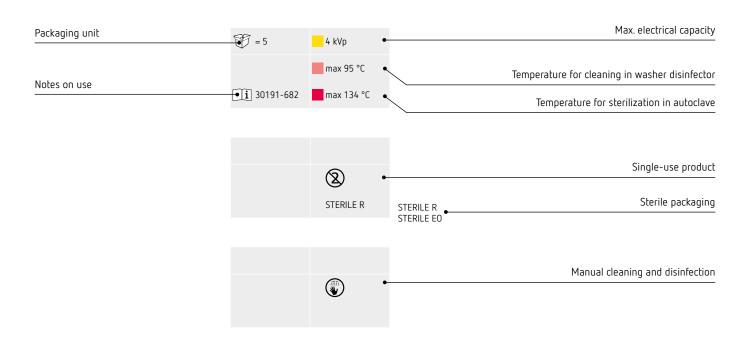

Please read carefully the corresponding notes on use before using any instrument.

Contents

Vessel sealing

Instruments and accessories

U	4	TriSect	rapide
---	---	---------	--------

04 BiClamp knife

05 BiClamp

13 BiClamp LAP forceps


17 BiClamp E LAP forceps


Accessories for treatment for BiClamp LAP and BiClamp E LAP forceps


erbe-med.com

TriSect rapide




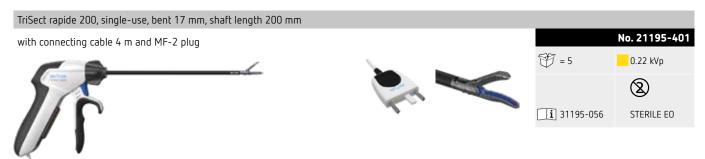

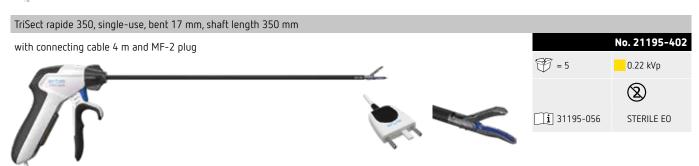

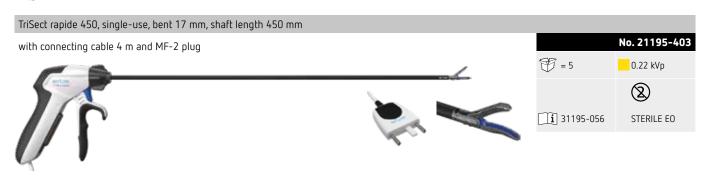

BiClamp knife

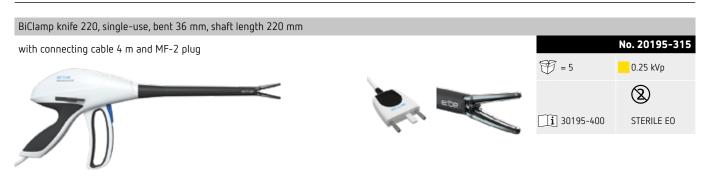

BiClamp








BiClamp




Product type	Length	Shape	Jaws	No.
BiClamp 150 C	150 mm	bent 23°	smooth	20195-221 21195-221
BiClamp 190 C	190 mm	bent 23°	smooth	21195-190
BiClamp 201 T	200 mm	bent 18°	smooth	20195-202 21195-202
BiClamp 210	210 mm	bent 25°	corrugated	20195-200 21195-200
BiClamp 260 C	260 mm	bent 18°	smooth	20195-299 21195-299
BiClamp 271 T	270 mm	bent 18°	smooth	20195-203 21195-203
BiClamp 280	280 mm	bent 25°	smooth	20195-280 21195-280

100 %

BiClamp

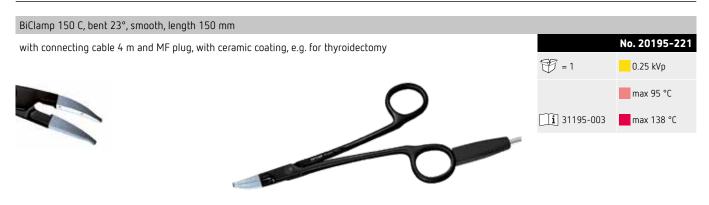


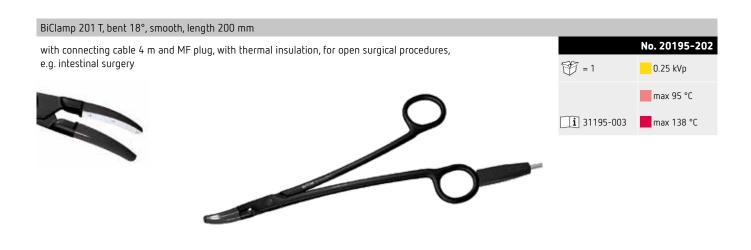





erbe-med.com


BiClamp

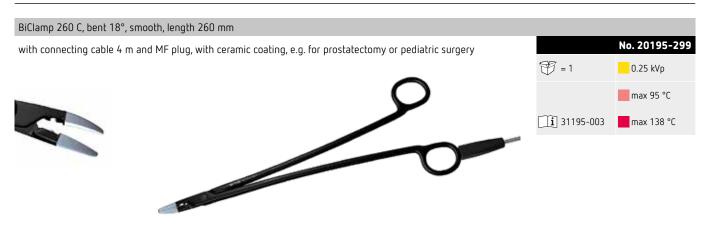


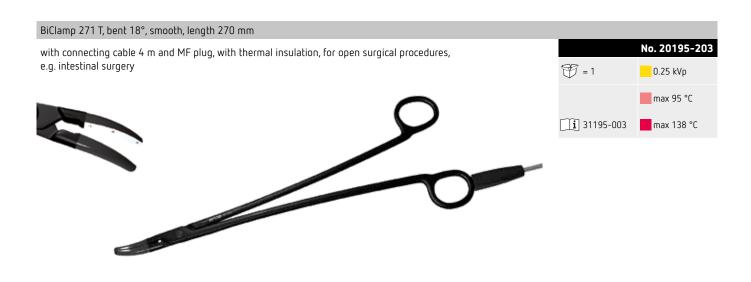


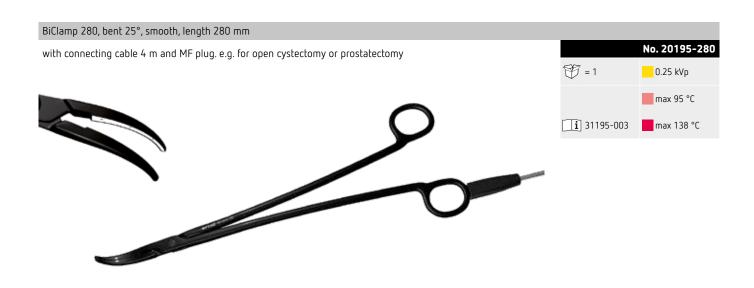

BiClamp

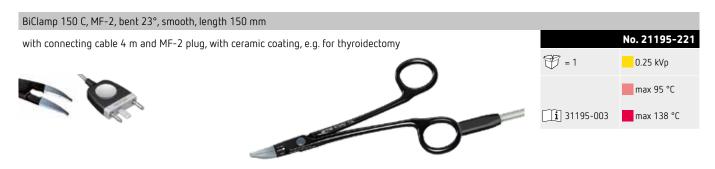

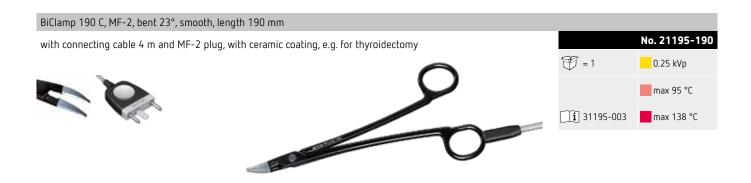


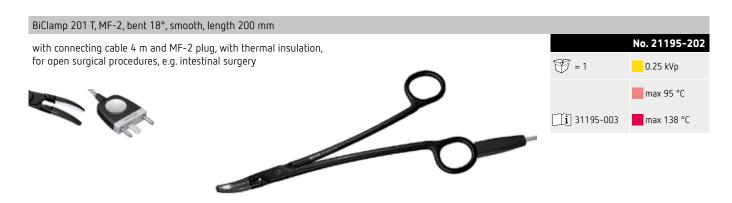





erbe-med.com

BiClamp

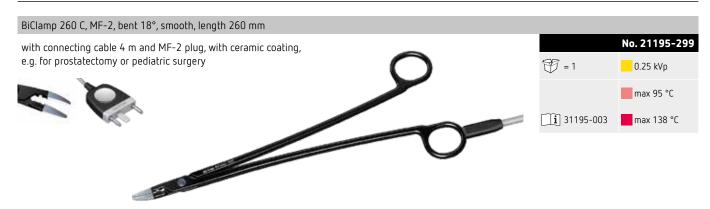

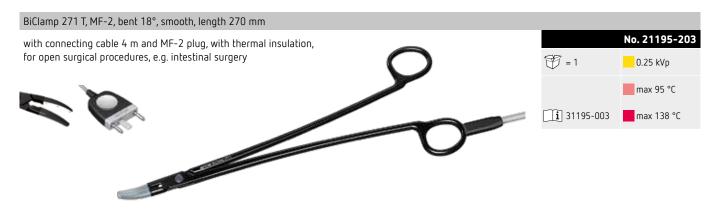

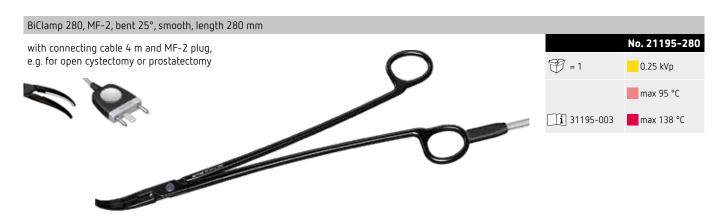

Adapters	Piece	No.
Adapter, MF-socket, MF-2-plug for VIO 300 D	1	20183-100
Adapter, MF-2/MF-U-socket, MF-plug for VIO 3 and VIO 300 D	1	20183-101

BiClamp LAP forceps










erbe-med.com

BiClamp LAP forceps





BiClamp LAP forceps

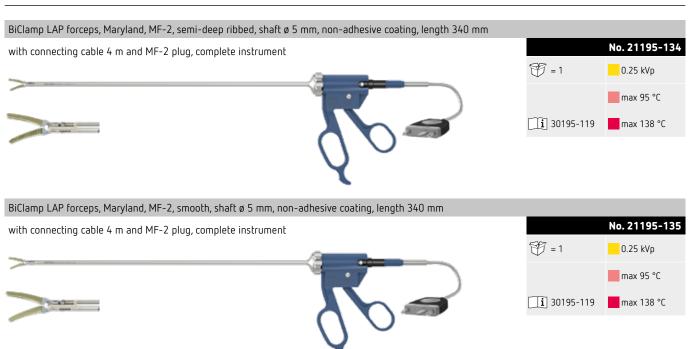







erbe-med.com


BiClamp LAP forceps



Single components		Piece	No.
Insert for BiClamp LAP forceps, Kelly, shaft ø 5 mm, length 340 mm (for 20195-228)	The spine of boxes	1	20195-236
Insert for BiClamp LAP forceps, Maryland, semi-deep ribbed, shaft ø 5 mm, length 340 mm (for 20195-134)	The section of	1	20195-146
Insert for BiClamp LAP forceps, Maryland, smooth, shaft ø 5 mm, length 340 mm (for 20195-135)	The sections	1	20195-147
Insert for BiClamp LAP forceps, fenestrated, semi-deep, shaft ø 5 mm, length 340 mm (for 20195-136)	and the same	1	20195-148
Insert for BiClamp LAP forceps, fenestrated, smooth, shaft ø 5 mm, length 340 mm (for 20195-137)	arba	1	20195-149
Insert for BiClamp 110, smooth, shaft ø 5 mm, length 110 mm (for 20195-230)	The section of	1	20195-232
Shaft tube for bipolar LAP forceps and BiClamp LAP forceps		1	20195-141
Shaft tube for BiClamp 110, ø 5 mm, length 110 mm (for 20195-230)		1	20195-234
Handle for BiClamp LAP forceps and BiClamp 110, with connecting cable 4 m and MF plug	160	1	20195-145
Handle for BiClamp LAP forceps and BiClamp 110, with connecting cable 4 m and MF-2 plug	160	1	21195-145

Adapters	Piece	No.
Adapter, MF-socket, MF-2-plug for VIO 300 D	1	20183-100
Adapter, MF-2/MF-U-socket, MF-plug for VIO 3 and VIO 300 D		20183-101

BiClamp E LAP forceps

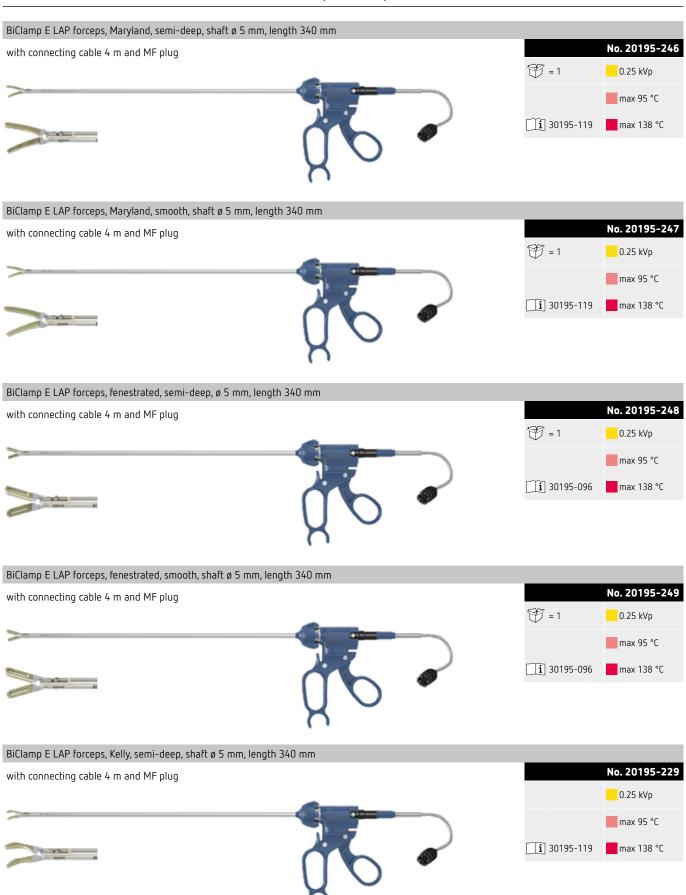

erbe-med.com

BiClamp E LAP forceps











BiClamp E LAP forceps

Single components		Piece	No.
Insert for BiClamp E LAP forceps, Kelly, shaft ø 5 mm, length 340 mm (for 20195-229, 21195-229)	erbe	1	20195-236
Insert for BiClamp E LAP forceps, Maryland, semi-deep ribbed, shaft ø 5 mm, length 340 mm (for 20195-246, 21195-246)	The section of the se	1	20195-146
Insert for BiClamp E LAP forceps, Maryland, smooth, shaft ø 5 mm, length 340 mm (for 20195-247, 21195-247)	The sections	1	20195-147
Insert for BiClamp E LAP forceps, fenestrated, semi-deep, shaft ø 5 mm, length 340 mm (for 20195-248, 21195-248)	arisa	1	20195-148
Insert for BiClamp E LAP forceps, fenestrated, smooth, shaft ø 5 mm, length 340 mm (for 20195-249, 21195-249)	arisa	1	20195-149
Shaft tube for BiClamp E LAP forceps, ø 5 mm, length 340 mm		1	20195-241
Handle for BiClamp E LAP forceps, with connecting cable 4 m and MF plug (for 20195-246, 20195-247, 20195-248, 20195-249, 20195-229)	g6.	1	20195-240
Handle for BiClamp E LAP forceps, with connecting cable 4 m and MF-2 plug (for 21195-246, 21195-247, 21195-248, 21195-249, 21195-229)	963	1	21195-240

Adapters	Piece	ce No.
Adapter, MF-socket, MF-2-plug for VIO 300 D		20183-100
Adapter, MF-2/MF-U-socket, MF-plug for VIO 3 and VIO 300 D		20183-101

Accessories for treatment for BiClamp LAP and BiClamp E LAP forceps

Accessories for treatment	Piece	No.
Cleaning brush for suction channel max. ø 3.5 mm, length 650 mm, for manual cleaning and disinfection	 1	20191-279
Irrigation tube for shaft tube with Luer Lock connector, length 500 mm, for LAP instruments, for cleaning and disinfection by machine	1	20195-201

erbe-med.com

Important information

The information, recommendations and other details contained in this medium ("information") reflect our state of knowledge and the state of the art in science and technology at the time the medium was created. The information is of a general nature, non-binding and intended solely for general information purposes; it does not constitute instructions for use.

The information and recommendations contained in this medium do not create any legal obligations on the part of Erbe Elektromedizin GmbH and its affiliated companies ("Erbe") or any other claims against Erbe. The information does not constitute any guarantees or other information on the nature of the product; such information requires an express contractual agreement with Erbe in each individual case.

Erbe is not liable for any kind of damage resulting from following the information on this medium, regardless of any legal grounds for liability.

Every user of an Erbe product is responsible for testing the respective Erbe product in advance with regard to its properties and its suitability for the intended type of use or purpose. Suitable type of use of the respective Erbe product can be found in the instructions for use for the respective Erbe product. The user is obliged to ascertain whether the instructions for use available to him/her correspond to the current status of the specific Erbe product. Devices may only be used in accordance with the instructions for use.

Information on settings, application sites, application duration and use of the respective Erbe product is based on the clinical experience of individual centers, physicians and clinical literature independent of Erbe as well as post market surveillance and empirical evidence. They constitute reference values, or Experienced Starting Settings, which must be checked by the user to ensure that they are suitable for the specifically planned application. Depending on the circumstances of a specific application, it may be necessary to deviate from the information provided. The user is responsible for checking this when using Erbe products. We wish to note that science and technology are subject to constant development as a result of research and clinical experience. Similarly, medicine and clinical application are constantly evolving as a result of research and technological development. This may also make it necessary for the user to deviate from the information provided on this medium.

This medium contains information about Erbe products that may not be approved/cleared in certain countries. The user of the respective Erbe product is obliged to inform himself/herself as to whether the Erbe product he/she is using is legally approved/cleared in his/her country and/or to what extent, if any, there are legal requirements for or restrictions on its use.

This medium is not intended for use in the USA

Erbe Elektromedizin GmbH Waldhoernlestrasse 17 72072 Tuebingen Germany

Phone +49 7071 755-0 info@erbe-med.com erbe-med.com medical-videos.com



